

CD16 Monoclonal Antibody (3G8), NovaFluor™ Blue 660-120S, eBioscience™

Product Details

Size	100 Tests
Species Reactivity	Baboon, Chimpanzee, Cynomolgus monkey, Human, Non-human primate, Rhesus monkey
Host/Isotype	Mouse / IgG1
Class	Monoclonal
Type	Antibody
Clone	3G8
Conjugate	NovaFluor™ Blue 660-120S
Excitation/Emission Max	492/665 nm
Form	Liquid
Concentration	4 µL/Test
Purification	Affinity chromatography
Storage buffer	PBS, pH 7.2
Contains	0.09% sodium azide
Storage conditions	4° C, store in dark, DO NOT FREEZE!

Applications

Tested Dilution

Publications

Flow Cytometry (Flow) 4 µL (0.6 µg)/test

-

Product Specific Information

Description: This 3G8 monoclonal antibody reacts with human and non-human primate CD16, which is also known as the low-affinity Fc gamma RIII. CD16 exists as two distinct isoforms, Fc gamma RIIIA and Fc gamma RIIIB. In humans, Fc gamma RIIIA is expressed as a polypeptide-anchored form on monocytes, macrophages, and lymphocytes such as NK cells. T and B cells do not express this Fc receptor. Fc gamma RIIIB is also detected on neutrophils as a GPI-anchored form. Expression of CD16 on lymphocytes and monocytes is similar in non-human primates. However, while CD16 is not found on neutrophils in macaques and baboons, this receptor is detected on these cells in sooty mangabeys. Binding of IgG leads to activation of signal transduction pathways, resulting in antibody-dependent cell-mediated cytotoxicity (ADCC), phagocytosis, cytokine release, and antigen presentation.

Based on cross-blocking studies 3G8 recognizes the same epitope as CB16. However, 3G8 and B73.1 antibody clones bind distinct epitopes.

Each product contains 1 vial of NovaFluor conjugate and 1 vial of CellBlox Plus Blocking Buffer .

Applications Reported: This 3G8 antibody has been reported for use in flow cytometric analysis.

Applications Tested: This 3G8 antibody has been pre-diluted and tested by flow cytometric analysis of normal human peripheral blood cells. This may be used at 4 µL (0.6 µg) per test. A test is defined as the amount (µg) of antibody that will stain a cell sample in a final volume of 100 µL. Cell number should be determined empirically but can range from 10⁵ to 10⁸ cells /test.


NovaFluor dyes are not compatible with DNA intercalating viability dyes. Do not use viability dyes such as propidium iodide, 7-actinomycin D (7-AAD) and DAPI. Invitrogen LIVE/DEAD Fixable Dead Cell stains are recommended for use with NovaFluor dyes.

This NovaFluor conjugate has been updated to ship with CellBlox Plus Blocking Buffer (Cat. No. (C001T06F01)). This buffer contains formulation improvements over CellBlox. CellBlox Plus Blocking Buffer is required for optimal staining with NovaFluor conjugates and should be used in all experiments where NovaFluor conjugates are used. Whenever possible, we recommend adding CellBlox Plus Blocking Buffer to antibody cocktails/master mixes prior to combining with cells. Add 5 µL per sample (regardless of the number of NovaFluors in your panel) to use the antibody cocktail as intended. For single-color controls, use 5 µL of CellBlox Blocking Buffer per 100 µL of cell sample containing 10³ to 10⁸ cells.

NovaFluor conjugates are based on Phiton™ technology utilizing novel nucleic acid dye structures that allow for engineered fluorescent signatures with consideration for spillover and spread impacts. Learn more


Excitation: 509 nm; Emission: 665 nm; Laser: 488 nm (Blue) Laser

Product Images For CD16 Monoclonal Antibody (3G8), NovaFluor™ Blue 660-120S, eBioscience™

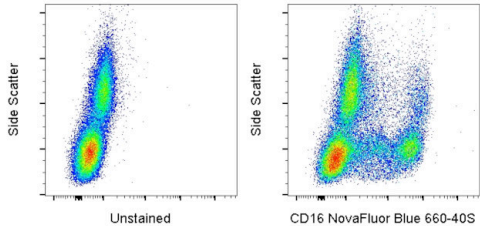


CD16 Antibody (H006T03B08-A) in Flow

Staining of normal human peripheral blood cells with side scatter and unstained (left) or CD16 Monoclonal Antibody, NovaFluor Blue 660-120S (right). Data was acquired in the B7 channel on a 5-laser Cytex Aurora and singlet cells were used for analysis.

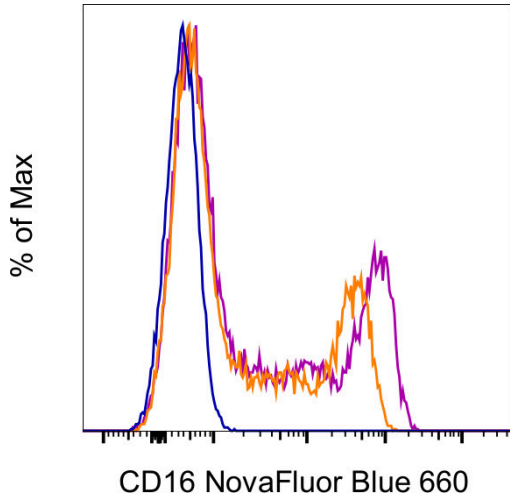

CD16 Antibody (H006T03B08-A) in Flow

Normal human PBMCs were either left unstained (blue histogram) or stained with CD16 Monoclonal Antibody, NovaFluor Blue 660-40S (orange histogram) or CD16 Monoclonal Antibody, NovaFluor Blue 660-120S (purple histogram) and acquired in the B7 channel on a 5-laser Cytex Aurora. Cells in the lymphocyte gate were used in the analysis.

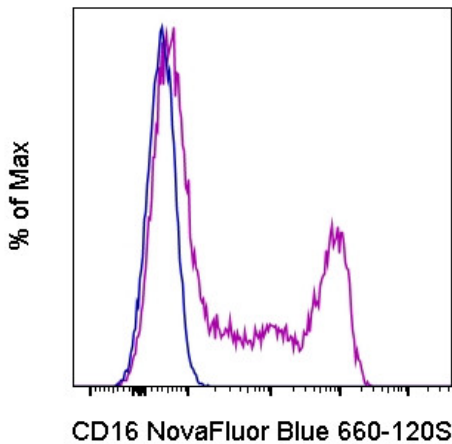

CD16 Antibody (H006T03B08-A) in Flow

Normal human peripheral blood cells were either left unstained (blue histogram) or stained with CD16 Monoclonal Antibody, NovaFluor Blue 660-120S (purple histogram) and acquired in the B7 channel on a 5-laser Cytex Aurora. Cells in the lymphocyte gate were used in the analysis.

View more figures on thermofisher.com

For Research Use Only. Not for use in diagnostic procedures. Not for resale without express authorization. Products are warranted to operate or perform substantially in conformance with published Product specifications in effect at the time of sale, as set forth in the Production documentation, specifications and/or accompanying package inserts ("Documentation"). No claim of suitability for use in applications regulated by FDA is made. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the Product is subjected to normal, proper and intended usage. This warranty does not extend to anyone other than the Buyer. Any model or sample furnished to Buyer is merely illustrative of the general type and quality of goods and does not represent that any Product will conform to such model or sample. NO OTHER WARRANTIES, EXPRESS OR IMPLIED, ARE GRANTED INCLUDING WITHOUT LIMITATION, IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR ANY PARTICULAR PURPOSE, OR NON INFRINGEMENT. BUYER'S EXCLUSIVE REMEDY FOR NON-CONFORMING PRODUCTS DURING THE WARRANTY PERIOD IS LIMITED TO REPAIR, REPLACEMENT OF OR REFUND FOR THE NON-CONFORMING PRODUCT(S) AT SELLER'S SOLE OPTION. THERE IS NO OBLIGATION TO REPAIR, REPLACE OR REFUND FOR PRODUCTS AS THE RESULT OF (I) ACCIDENT, DISASTER OR EVENT OF FORCE MAJEURE, (II) MISUSE, FAULT OR NEGLIGENCE OF OR BY BUYER, (III) USE OF THE PRODUCTS IN A MANNER FOR WHICH THEY WERE NOT DESIGNED, OR (IV) IMPROPER STORAGE AND HANDLING OF THE PRODUCTS. Unless otherwise expressly stated on the Product or in the documentation accompanying the Product, the Product is intended for research only and is not to be used for any other purpose, including without limitation, unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to human or animals.